

FIG.I
INS ENVIRONMENT

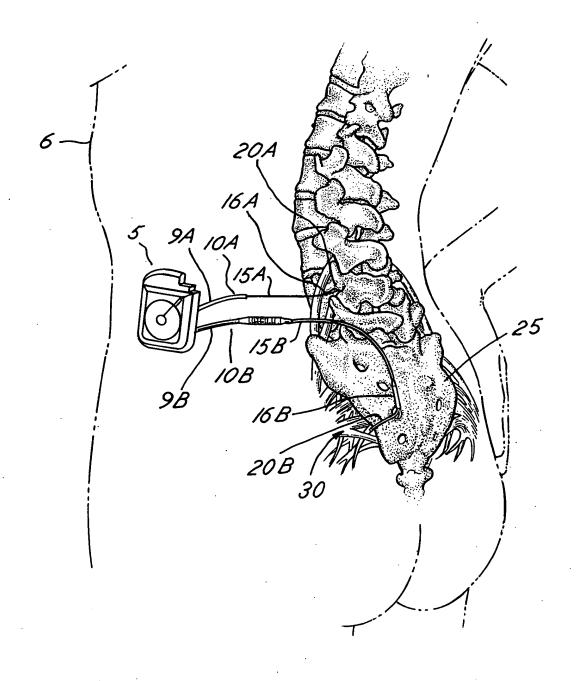
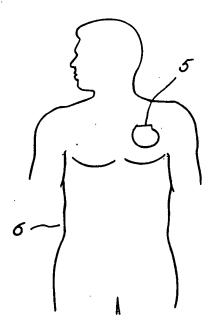




FIG. 2A











FIG.2C


FIG.2D



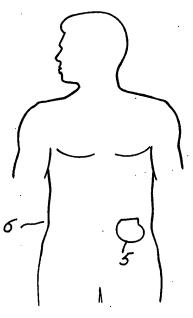

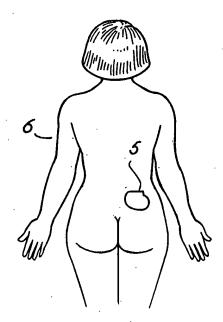

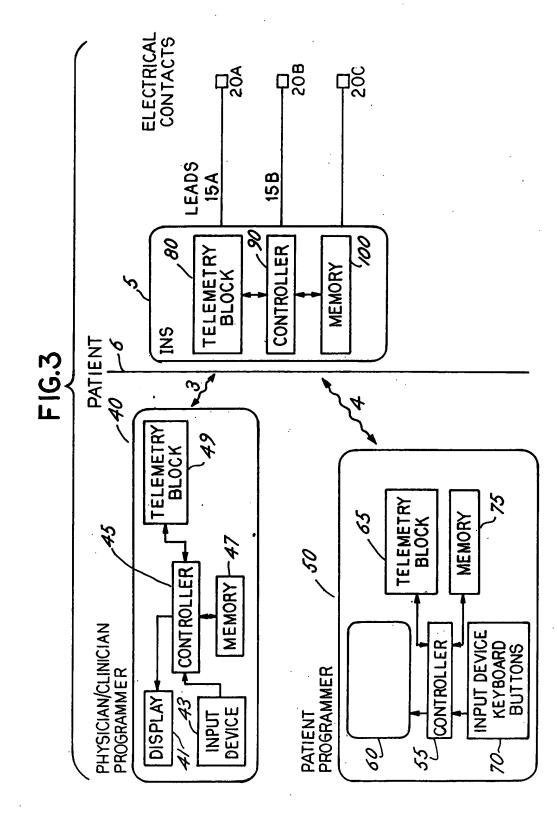

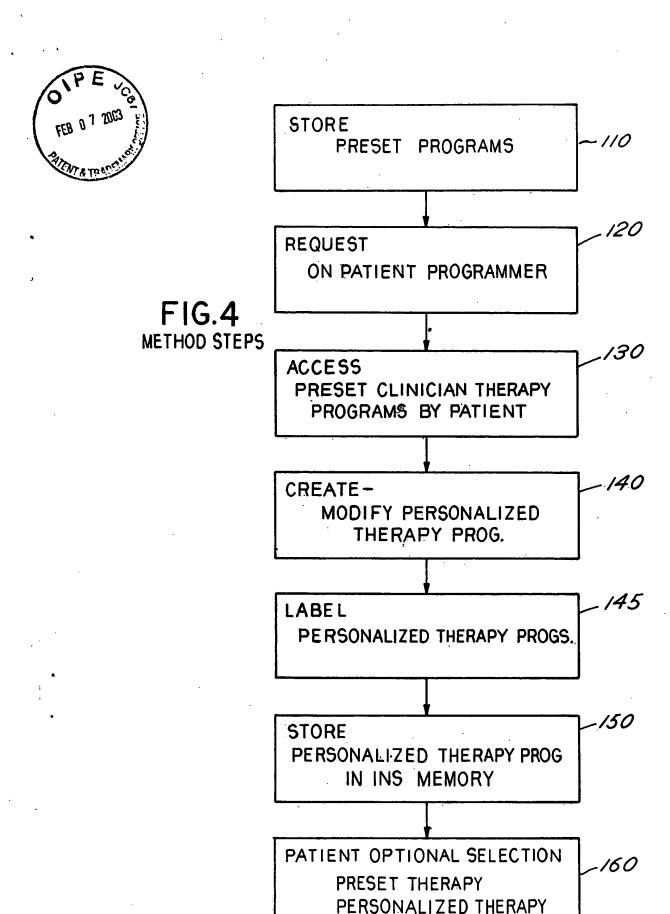



THERAPY SETTINGS (PCTS) -ELECTRODE POLARITIES -DIRECTIONAL SEQUENCE -PULSE WÍDTH MIN/MAX -AMPLITUDE MIN/MAX -RATE MIN/MAX PRESET CLINICIAN THERAPY PROGRAMS (PCTP) **PROGRAMS** 4 F 2 ಔ 2 PATIENTS BUILDS
/#0~ACTIVITY SETS AMPL RATE PW AMPL RATE PW AMPL RATE PW AMPL RATE PW P4 AMPL RATE PW /90 PROGRAMS/SETTINGS **P3** 집 5 AMPL RATE PW AMPL RATE PW 200-2/0 AMPL RATE PW "SITTING" "SLEEP" OTHER 220